



ATD – GCMS for BTX/ VOCs

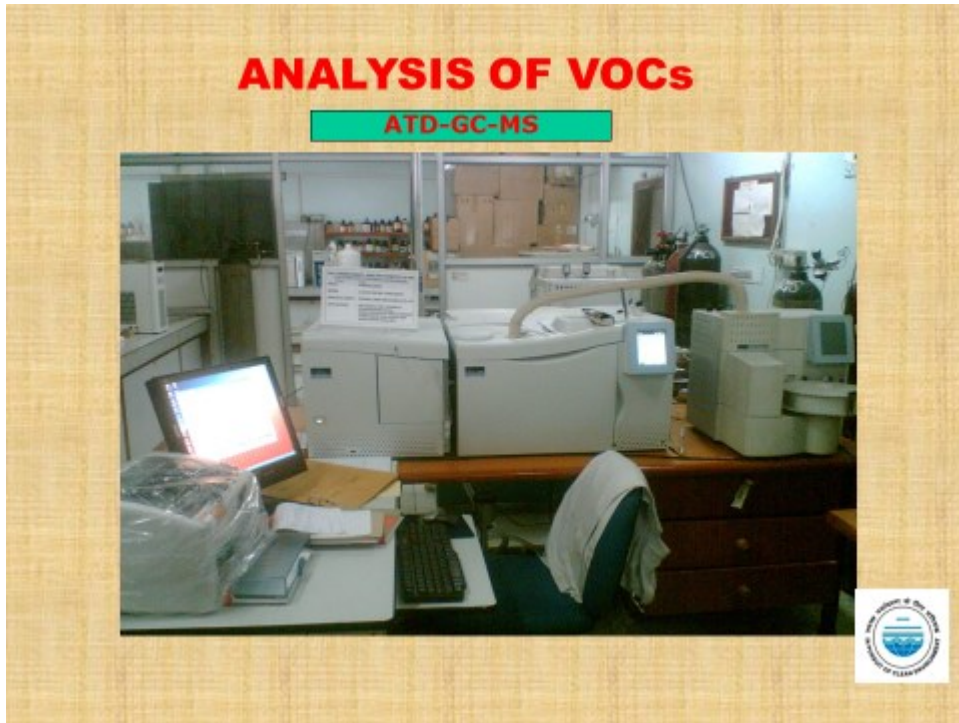

Sampling Devices for BTX/ VOCs

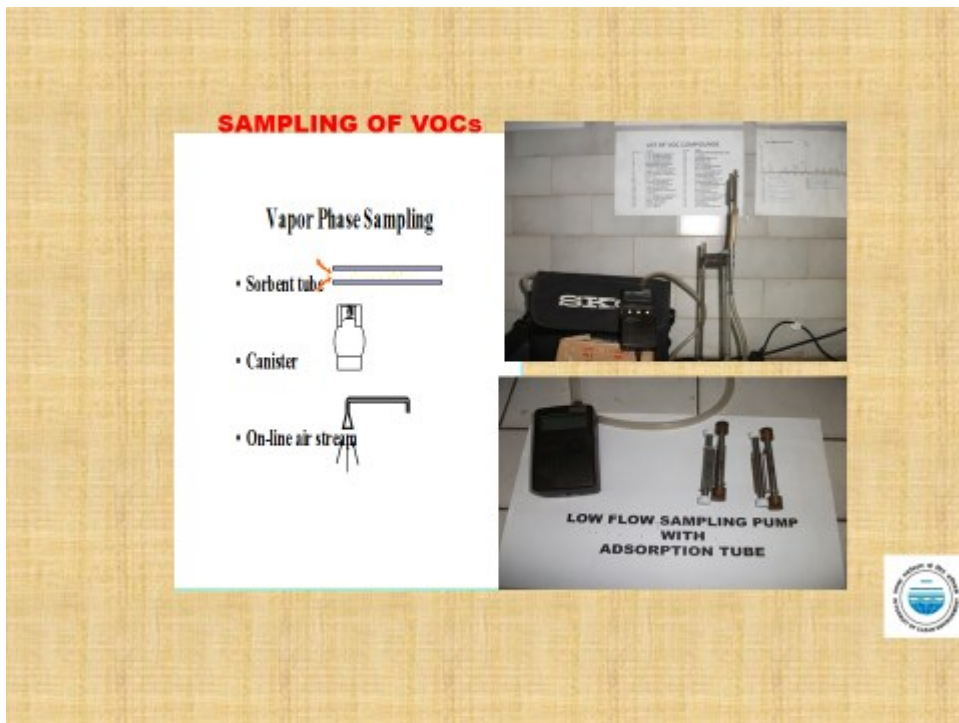

ACTIVE SAMPLING TUBES: Glas/Activated Charcoal & SS Tenex A



Rotary Evaporator for Concentration of PAHs Extract



GC – FID for PAHs Analysis

